




# Pituitary Rongeur with Teeth

Designed by Michael Murray, MD

*Designed to optimize the efficiency of soft tissue removal and disc space preparation prior to a spinal interbody fusion*

Unique design ensures that only the distal tip of the instrument is in contact upon closure of the jaws, allowing the grasping force to be optimized, and directed at the distal tip of the instrument. In addition, the teeth at the distal end of the instrument allow for a better grasp on tissues or disc material, for enhanced control and efficiency of removal.

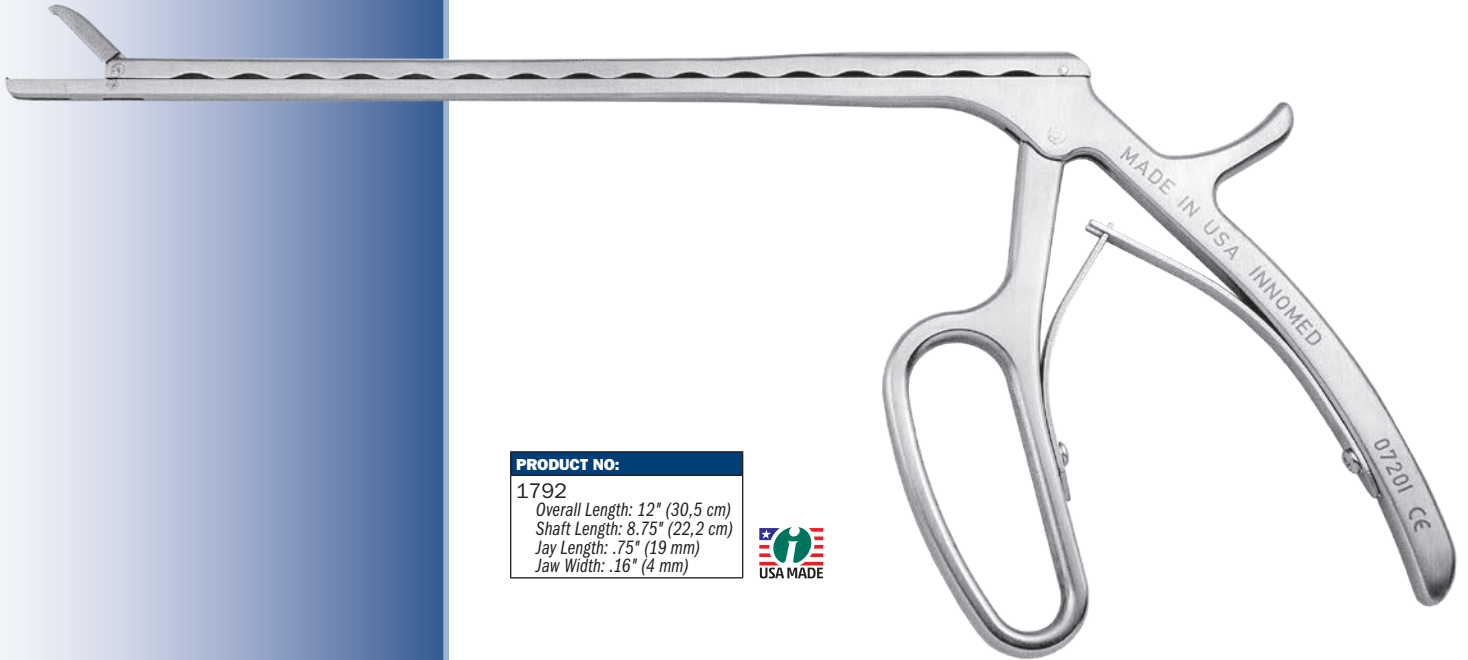

**PRODUCT NO:**

1792  
Overall Length: 12" (30,5 cm)  
Shaft Length: 8.75" (22,2 cm)  
Jaw Length: .75" (19 mm)  
Jaw Width: .16" (4 mm)



ISO 13485:2016

**FREE TRIAL ON MOST INSTRUMENTS**

Scan to  
Launch Our  
Website



103 Estus Drive, Savannah, GA 31404  
www.innomed.net info@innomed.net

912.236.0000 Phone  
912.236.7766 Fax

Innomed-Europe Tel. +41 41 740 67 74  
Fax +41 41 740 67 71

**INNOMED**

**1.800.548.2362**